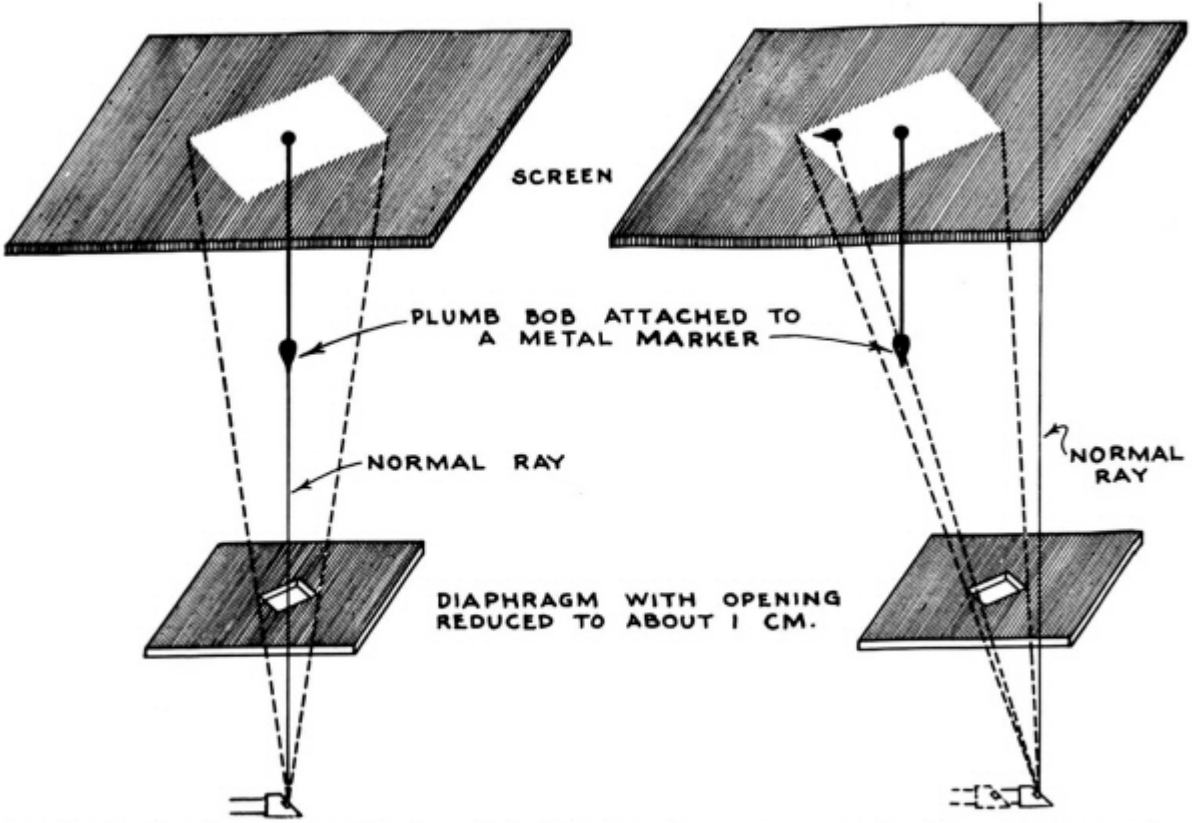

FIG. 110.—Showing the positions of shadow of plumb bob on fluorescent screen when X-ray tube is properly centered, and when off center