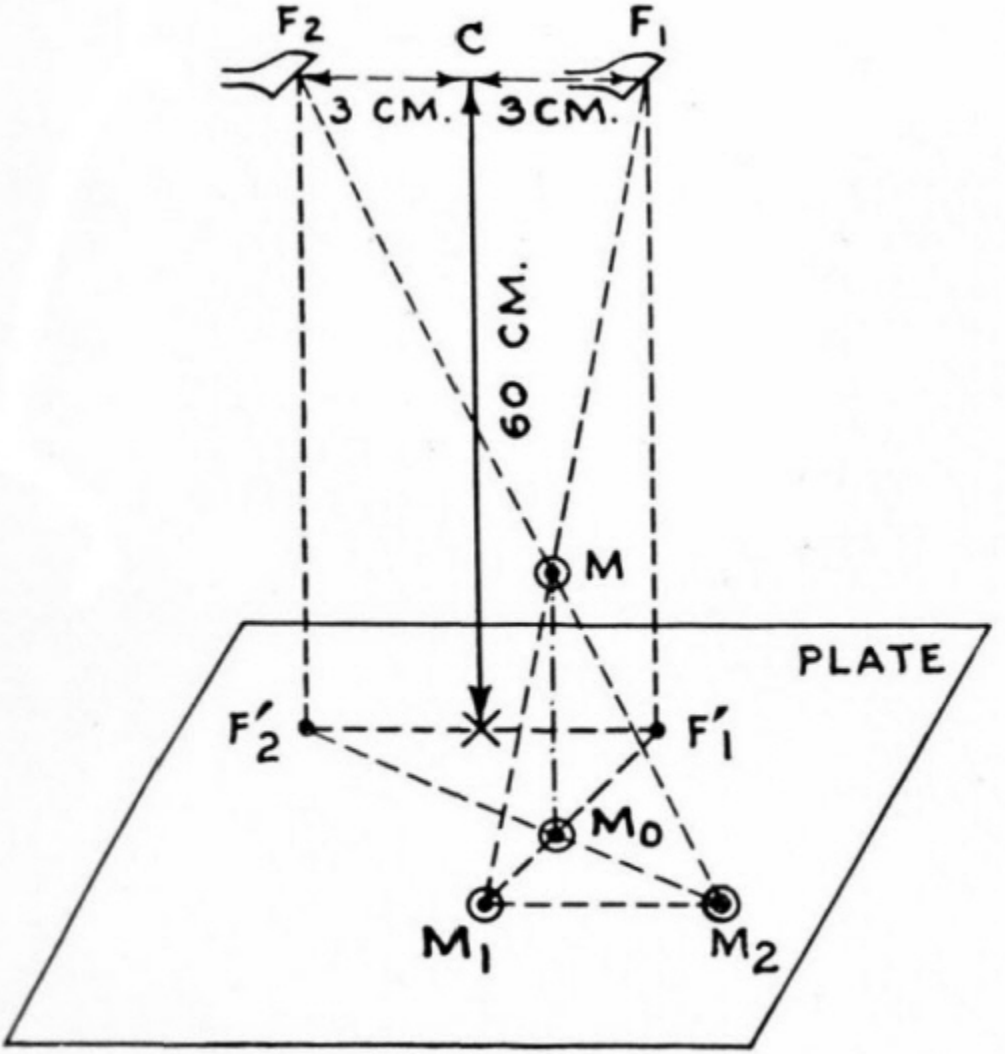

FIG. 143.—Schematic representation of plate, cross-wire marker, and tube focus positions for radiographic use of Hirtz compass