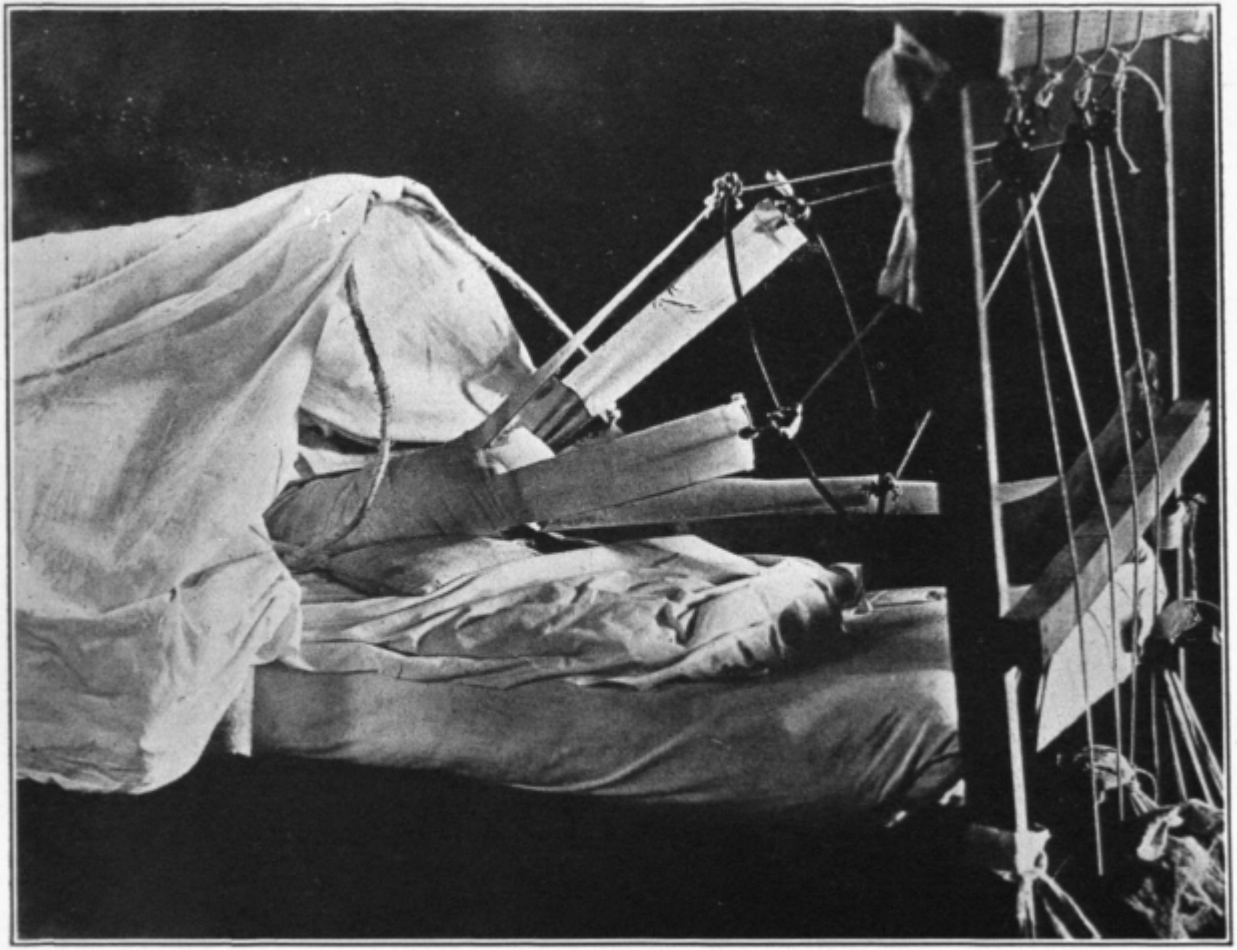

FIG. 130.—Use of a spreader in sliding extension applied to an amputation stump to overcome soft part retraction